



LAWRENCE
LIVERMORE
NATIONAL
LABORATORY

A novel heterodyne displacement interferometer with no detectable periodic nonlinearity and optical resolution doubling

K. Joo, J. D. Ellis, E. S. Buice, J. W. Spronck, R. H. Munnig Schmidt

February 11, 2010

10th International Conference of the European Society for
Precision Engineering and Nanotechnology
Deft, Netherlands
May 31, 2010 through June 4, 2010

Disclaimer

This document was prepared as an account of work sponsored by an agency of the United States government. Neither the United States government nor Lawrence Livermore National Security, LLC, nor any of their employees makes any warranty, expressed or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States government or Lawrence Livermore National Security, LLC. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States government or Lawrence Livermore National Security, LLC, and shall not be used for advertising or product endorsement purposes.

A novel heterodyne displacement interferometer with no detectable periodic nonlinearity and optical resolution doubling

Ki-Nam Joo¹, Jonathan D. Ellis¹, Eric S. Buice^{1,2}, Jo. W. Spronck¹, Robert H. Munnig Schmidt¹

¹*PME: Mechatronic System Design, Delft University of Technology, The Netherlands*

²*As of 19-01-10 at Lawrence Livermore National Laboratory, Livermore, USA*

Corresponding k.joo@tudelft.nl, J.W.Spronck@tudelft.nl

Abstract

This paper describes a novel heterodyne laser interferometer with no significant periodic nonlinearity for linear displacement measurements. Moreover, the optical configurations have the benefit of doubling the measurement resolution when compared to its respective traditional counterparts. Experimental results show no discernable periodic nonlinearity for a retro-reflector interferometer and plane mirror interferometer configurations with a noise level below 20 pm. The incoming laser beams of the interferometers are achieved by utilizing two single mode optical fibers. To determine the stability of the optical fiber couplers a fiber delivery prototype was also built and tested.

1 Introduction

Eliminating periodic nonlinearity in heterodyne laser interferometry has been the subject of much research, which can be categorized as either algorithm methods [1] or two spatially separated beam interferometer configurations [2]. The reduction method algorithms ensure a periodic nonlinearity below 1 nm without changes to the interferometer configurations; however, they typically require a calibration period, a nominal velocity, and additional calculation time. Conversely, real time reductions can be implemented with modified interferometer setups using two spatially separated beams. The only limitation of these configurations is their special and often complicated configurations which limit their applicability in industrial fields.

In this research, we propose two simple heterodyne interferometer configurations, with retroreflector and with plane mirror targets, with two spatially separated beams to eliminate the periodic nonlinearity. The optical resolution doubling allows for

simpler optical configurations while achieving the same optical resolution by increasing the number of beam paths in the interferometer.

2 A novel heterodyne laser interferometer without periodic nonlinearity

2.1 Basic concept

The interferometer, as shown in Fig.1(a), consists of a beam splitter (BS), a right angle prism (RAP) as the reference mirror, and a retro-reflector (RR) as the moving target.

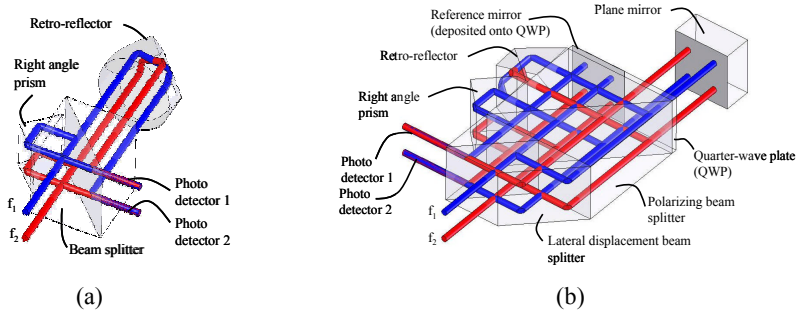


Figure 1: Optical configuration of a novel heterodyne laser interferometer; (a) retro-reflector and (b) plane mirror type.

Two parallel beams from the optical source (f_1 and f_2) travel to the BS and the reflected beams travel toward the RAP, which has line symmetry. The transmitted beam travels to the RR, which has point symmetry [3]. Then, the reference and measurement beams can be recombined by the BS to create an interference with opposite phase directions, detected by the photodetectors (PD_1 and PD_2). From the PD_1 and PD_2 , the phase difference $\varphi = 8\pi\Delta L/\lambda$ (where ΔL is the displacement of the RR and λ is the wavelength of light), which results in an optical resolution of $\lambda/4$.

For the plane mirror applications, the two parallel beams are divided by a linear displacement beam splitter (LDBS) into two sets, reference beams and measurement beams as shown in Fig.1(b). Similar to a typical plane mirror interferometer, each set of beams has the double-path between a polarizing beam splitter (PBS) and mirrors. The measurement beams are reflected by a RR experiencing the point symmetry while the reference beams have the line symmetry with a RAP. The two sets of beams propagate back to the LDBS and are then recombined to make the heterodyne signals.

In this interferometer, the optical resolution is $\lambda/8$ because of the double-path interferometer setup.

2.2 Experimental results

To evaluate the periodic nonlinearity, the measured displacements were fitted with a second order polynomial and the difference between the measured displacements and fitted displacements was applied to a fast Fourier transform (FFT) to detect the periodicity [4]. Figure 2 presents the periodic nonlinearity of the both interferometer types according to the fringe order in the FFT domain compared to the typical interferometers. As shown in Fig.2(a), the periodic nonlinearity in the retro-reflector interferometer was below the noise level, of approximately 20 pm, while the periodicity for the typical interferometer using a Zeeman laser was determined to be approximately 7 nm at the first fringe order. Similar to the retro-reflector interferometer case, no periodic nonlinearity was detected with the plane mirror configuration, while a commercial interferometer (E1826G, Agilent) has the first order nonlinearity of approximately 0.3 nm, see Fig.2(b). While no periodic nonlinearity is detectable with the proposed interferometer at half, first and second fringe order, however, several peaks appeared in the Fig.2. Those peaks are caused by the residual vibration effects from the stage motion after averaging and resolution limitations of the phase measuring electronics.

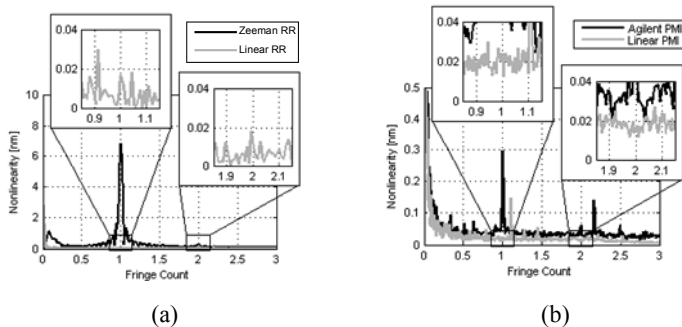


Figure 2: Periodic nonlinearity; (a) retro-reflector and (b) plane mirror type.

3 Prototype: fiber coupling module

For the next generation of beam delivering system, the fiber coupled interferometer module was designed with the basic concept of two spatially separated beams as depicted in Fig.3(a). Compared to the typical system using polarization maintaining

fibers, single mode fibers aligned with kinematic mounts were used for the beam delivery due to the polarization insensitivity. The position of the beam in plane was measured with a position sensitive detector (PSD) to evaluate the stability. Figure 3(b) shows the stability test result and displacements during 2.7 hours. They were 1.5 mrad and 100 nm for the PV values, respectively, mainly caused by the thermal expansion of the base steel plate. Improvements for the stability are still going on.

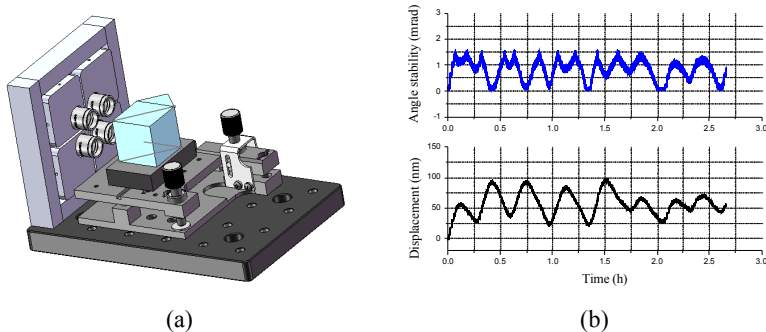


Figure 3: Prototype of interferometer module for optical fiber delivery system; (a) the configuration and (b) stability test result with displacements.

4 Conclusion

In this paper, we described two simple heterodyne interferometer configurations with two spatially separated beams to eliminate the periodic nonlinearity. In addition, the optical resolution was enhanced by a factor of two. The experimental results show the periodic nonlinearity was below the noise level of 20 pm. For industrial applications, a fiber delivered module was also considered and tested.

This work was supported by the Dutch IOP (projects IPT06104 and IPT04001) in the Netherlands. The authors would like to acknowledge Agilent Technologies and VSL Dutch Metrology Institute for their equipment support.

Lawrence Livermore National Laboratory is operated by Lawrence Livermore National Security LLC, for the U.S. Department of Energy, National Nuclear Security Administration under Contract DE-AC52-07NA27344. LLNL-PROC-423527

References:

- [1] D. Chu *et al.*, Proc. of 4th euspen Int. Conf., 300-301 (2004).
- [2] C. Wu *et al.*, Appl. Opt. **38**, 4089-4094 (1999).
- [3] K. -N. Joo *et al.*, Opt. Lett. **34**, 386-388 (2009).
- [4] K. -N. Joo *et al.*, Opt. Express. **18**, 1159-1165 (2010)